























#### Features

- 5"×3" compact size
- · 320W convection,500W force air
- 550W peak power (3sec.)
- Medical safety approved (2 x MOPP) accreding to ANSI/AAMI ES60601-1 and IEC/EN60601-1
- EMI for both Class I & Class II configuration
- -30~+70°C wide range operating temperature
- No load power consumption<0.5W by PS\_ON control</li>
- · High efficiency up to 94%
- Protections: Short circuit / Overload / Over voltage / Over temperature
- 5Vdc standby output, 12Vdc fan supply, Power Good, Power Fail and remote sense
- Operating altitude up to 4000 meters (Note.5)
- · LED indicator for power on
- · 3 years warranty




### Applications

- · Oral irrigator
- · Hemodialysis machine
- Medical computer monitors
- · Sleep apnea devices
- · Pump machine
- · Electric bed

### Description

RPS-500 is a 500W highly reliable green PCB type medical power supply with a high power density on the 5" by 3" footprint. It accepts 80~264VAC input and offers various output voltages between 12V and 48V. The working efficiency is up to 94% and the extremely low no load power consumption is down below 0.5W.RPS-500 is able to be used for both Class I (with FG) and Class II (no FG) system design. The extremely low leakage current is less than 220 µA. In addition, it conforms to international medical regulations (2\*MOPP) and EMC EN55011, perfectly fitting all kinds of BF rated "patient contact" medical system equipment. RPS-500 series also offers the enclosed style models (-C / TF /SF)

### Model Encoding



Туре	Description	Note
Blank	PCB Type	In stock
-C	Enclosed casing Type	In stock
-TF	Enclosed Type with fan on the top	In stock
-SF	Enclosed Type with fan on the side	In stock



SPECIFIC MODEL	AIION			RPS-500-12	RPS-500-15	RPS-500-18	RPS-500-24	RPS-500-27	RPS-500-36	RPS-500-48
MODEL	DC VOLTA	GF		12V	15V	18V	24V	27V	36V	48V
	DO VOLIA	OL .	25CEM							
	DATES	Blank	25CFM	41.6A	33.3A	27.8A	20.8A 13.4A	18.5A	13.9A	10.4A 6.7A
	RATED CURRENT		Convection	26.7A	21.3A	17.8A		11.9A	8.9A	
	Note.7	- c	25CFM	41.6A	33.3A	27.8A	20.8A	18.5A	13.9A	10.4A
			Convection	25.8A	20.7A	17.2A	12.9A	11.5A	8.6A	6.5A
		-TF/SF		41.6A	33.3A	27.8A	20.8A	18.5A	13.9A	10.4A
		Blank	25CFM Convection	499.2W	499.5W	500.4W	499.2W	499.5W	500.4W	499.2W 321.6W
	RATED POWER			320.4W 499.2W	319.5W	320.4W	321.6W	321.3W	320.4W	
	Note.7	- c	25CFM Convection	309.6W	499.5W 310.5W	500.4W 309.6W	499.2W 309.6W	499.5W 310.5W	500.4W 309.6W	499.2W 312W
		TE/0E			499.5W	509.6W	499.2W	499.5W	509.6W	499.2W
	DE 414 DOM	-TF/SF	Built-in fan	499.2W	433.300	300.477	433.200	433.300	300.477	433.200
	PEAK POV		•	550W 200mVp-p	200m\/n n	200m\/n n	200m\/n n	200mVp-p	200mVp-p	200mVp-p
OUTPUT	RIPPLE & N	•	,		200mVp-p	200mVp-p	200mVp-p			
			(main output)		14.3~15.8V	17.1~18.9V	22.8~25.2V	25.6 ~ 28.4V	34.2~37.8V	45.6 ~50.4V
	VOLTAGE T			±3.0%	±3.0%	±3.0%	±2.0%	±2.0%	±1.0%	±1.0%
	LINE REGU			±0.5%	±0.5%	±0.5%	±0.5%	±0.5%	±0.5%	±0.5%
	LOAD REGULATION		±1.0%	±1.0%	±1.0%	±1.0%	±1.0%	±1.0%	±1.0%	
	SETUP, RISE TIME		1000ms, 30ms		500ms, 30ms/1	15VAC at full loa	d			
	HOLD UP TIME (Typ.)			10ms/230VAC 10ms/115VAC at full load						
	VOLTAGE RANGE Note.4			80 ~ 264VAC 113 ~ 370VDC						
FREQUENCY RANGE 47 ~ 63Hz					′∼63Hz					
	POWER FACTOR			PF>0.94/230VAC PF>0.98/115VAC at full load						
INPUT	EFFICIENCY (Typ.)			91%	92%	92.5%	93%	93.5%	94%	94%
	AC CURRENT (Typ.)			5.8A/115VAC 2.9A/230VAC						
	INRUSH C	JRREN1	(Typ.)	COLD START 40A/115VAC 80A/230VAC						
	LEAKAGE CUI	RRENT (m	ax.) Note.5	Earth leakage current < 220 $\mu$ A/264 VAC 50Hz , Touch current < 100 $\mu$ A/264 VAC						
	OVEDLOA	<u> </u>		105 ~ 135% ra	ted output powe	r				
	OVERLOA	ט		Protection type: Hiccup mode, recovers automatically after fault condition is removed						
PROTECTION				13.2 ~ 15.6V   16.5 ~ 19.5V   19.8 ~ 23.4V   26.4 ~ 31.2V   29.7 ~ 35.1V   39.6 ~ 46.8V   52.8 ~ 62.4V						
	OVER VOL	TAGE		Protection type	: Shut down o/p	voltage, re-pov	ver on to recover			
	OVER TEN	IPERAT	URE	Protection type: Shut down o/p voltage, recovers automatically after temperature goes down						
				5Vsb: 5V@0.6A without fan, 1A with fan 25CFM;						
	5V STANDI	ВҮ		Tolerance ±2%, ripple : 120mVp-p(max.)						
				12V@0.5A for driving fan ;						
	12V FAN S	UPPLY		Tolerance ±10%						
FUNCTION				Power ON: PS-ON = "Hi" or " > 2 ~ 5V";						
	PS-ON INP	UT SIGI	IAL	Power ON: PS-ON = HI or >2~5V; Power OFF: PS-ON = "Low" or " < 0 ~ 0.5V"						
				500ms>PG>10ms; The TTL signal goes high with 10ms to 500ms delay after power set up;						
POWER GOOD / POWER FAIL			The TTL signal goes low at least 1ms before Vo below 90% of rated value							
	WORKING TEMP.			-30 ~ +70°C (Refer to "Derating Curve")						
				20 ~ 90% RH non-condensing						
ENVIDONMENT	WORKING HUMIDITY STORAGE TEMP.			-40 ~ +85°C	.en condending					
FIRMINORMENT	TEMP. COE		NT	±0.03%/°C (0	) ~ 50°C \					
	VIBRATION		11	,		e, 60min. each a	along X V 7 av	26		
	OPERATING		DE Note.6	*	o rommi./ reyer	o, oomin. Bacili	anony A, I, Z dXt			
	OI LIVATING	ALITIUL	- Note.0	4000 meters						



#### **SPECIFICATION**

	SAFETY STANDARDS	IEC60601-1, TUV EN UL ANSI/AAMI ESG CAN/CSA-C22.2 No Design refer to E	60601-1 (3.1 ve . 60601-1:14 - E	Edition	3 approved;				
	ISOLATION LEVEL	Primary-Secondary:	imary-Secondary: 2xMOPP, Primary-Earth:1xMOPP, Secondary-Earth:1xMOPP						
	WITHSTAND VOLTAGE	I/P-O/P:4KVAC I/P	-FG:2KVAC	O/P-FG	:1.5KVAC				
	ISOLATION RESISTANCE	I/P-O/P, I/P-FG:100I	/P-O/P, I/P-FG:100M Ohms / 500VDC / 25°C/ 70% RH						
		Parameter		Stand	ard		Test Level / N	lote	
		Conducted emission		EN55011 (CISPR11)			Class I : Class	s B , Class II : Class A	
	EMC EMISSION	Radiated emission		EN550	)11 (CISPR11)		Class A		
SAFETY &		Harmonic current		EN610	000-3-2		Class A		
EMC		Voltage flicker		EN610	000-3-3				
(Note 8)		EN55024 , EN60601-1-2, EN61204-3							
		Parameter		Standard		Test Level / Note			
		ESD		EN61000-4-2		Level 4, 15KV air ; Level 4, 8KV contact			
		RF field susceptibility		EN61000-4-3		Level 3, 10V/m( 80MHz~2.7GHz ) Table 9, 9~28V/m( 385MHz~5.78GHz )			
	EMC IMMUNITY	EFT bursts		EN61000-4-4		Level 3, 2KV			
		Surge susceptibility		EN61000-4-5		Level 4, 4KV/Li	ne-FG ; 2KV/Line-Line		
		Conducted susceptibility		EN610	000-4-6		Level 3, 10V		
		Magnetic field immunity		EN61000-4-8		Level 4, 30A/r	n		
		Voltage dip, interruption		EN61000-4-11		100% dip 1 periods, 30% dip 25 periods, 100% interruptions 250 periods			
	MTBF	194.1Khrs min. MI	L-HDBK-217F	(25°C)					
	DIMENSION	Туре	RPS-500		RPS-500-C	RPS-	500-TF	RPS-500-SF	
	DIWENSION	1 *\A/*11	127x76.2x40n	nm	130x86x43mm	130x8	6x66.5mm	160x86x43mm	
OTHERS		L*W*H	5"x3"x1.57"in	inch 5.11"x3.39"x1.69"inch 5.11"x		3.39"x2.62"inch	6.3"x3.39"x1.69"inch		
		P.W.	0.46Kg		0.54Kg	0.58K	g	0.64Kg	
	PACKING	Q'TY	30pcs		24pcs	24pc	S	24pcs	
	FACRING	G.W.	14.8Kg		14Kg	14.9K	g	16.4Kg	
		M'MENT	1.03CUFT		0.77CUFT	0.860	CUFT	0.91CUFT	

- 1. All parameters NOT specially mentioned are measured at 230VAC input, rated load and 25 of ambient temperature.
- 2. Ripple & noise are measured at 20MHz of bandwidth by using a 12" twisted pair-wire terminated with a 0.1 \( \mu \) f & 47 \( \mu \) f parallel capacitor.
- 3. Tolerance: includes set up tolerance, line regulation and load regulation.
- 4. Derating may be needed under low input voltages. Please check the derating curve for more details.
- 5. Touch current was measured from primary input to DC output.


#### NOTE

- 6. The ambient temperature derating of 3.5°C/1000m with fanless models and of 5°C/1000m with fan models for operating altitude higher than 2000m(6500ft).
- 7. Please refer to "Derating curve".
- 8. The power supply is considered a component which will be installed into a final equipment. All EMC tests are executed by mounting the unit on a 360mm\*360mm metal plate with 1mm of thickness. The final equipment must be re-confirmed that it still meets EMC directives. For guidance on how to perform these EMC tests, please refer to "EMI testing of component power supplies." (as available on http://www.meanwell.com).


EMI Performance	Conducted	Radiated
Class I (with FG)	Class B	Class A
Class II (no FG)	Class A	Class A

#### ■ Block Diagram

PFC fosc: 90KHz PWM fosc: 100KHz

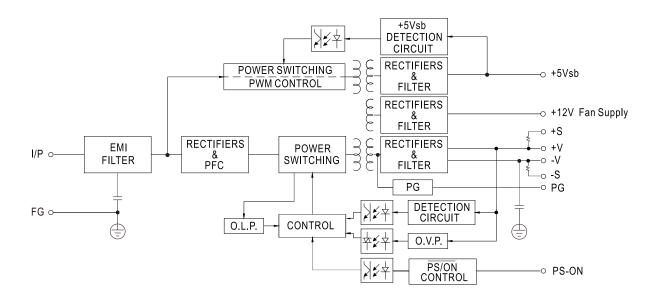


#### ■ Output Derating vs Input Voltage

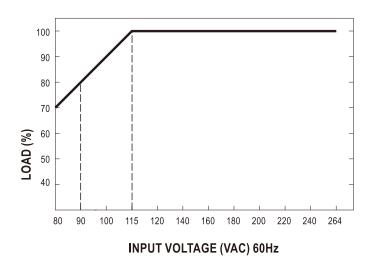




# ■ Derating Curve

### RPS-500

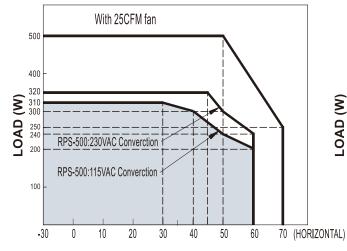


#### RPS-500-C

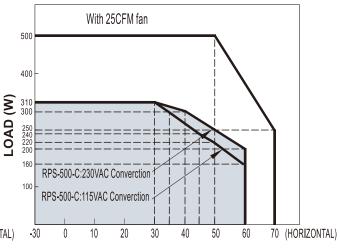

AMBIENT TEMPERATURE (°C)

#### AMBIENT TEMPERATURE (°C)

#### RPS-500-TF/SF

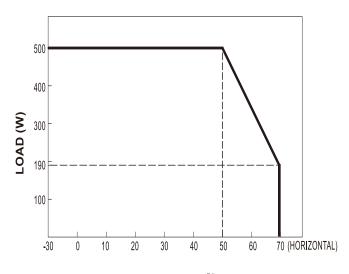



AMBIENT TEMPERATURE ( $^{\circ}$ C)


Order No.	RPS-500	RPS-500-C	RPS-500-TF	RPS-500-SF
Products			The state of the s	
Convection	320W	310W		
Force Air	500W	500W	500W	500W

## ■ Mechanical Specification RPS-500 (PCB Type) 127 <u>5.</u>6 115.8 CN95 31 42 Ф-HS4 21 LV -V $\overset{\perp}{\top}$ HS3 HS2 64.8 CN1 Air flow direction 25CFM FAN 3.0 max 43 40



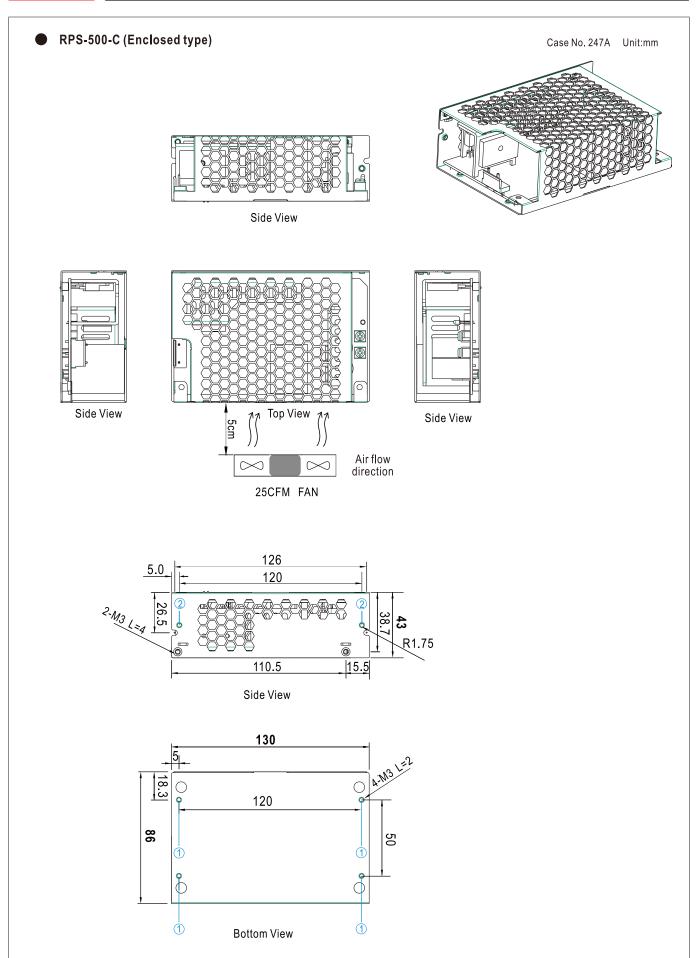

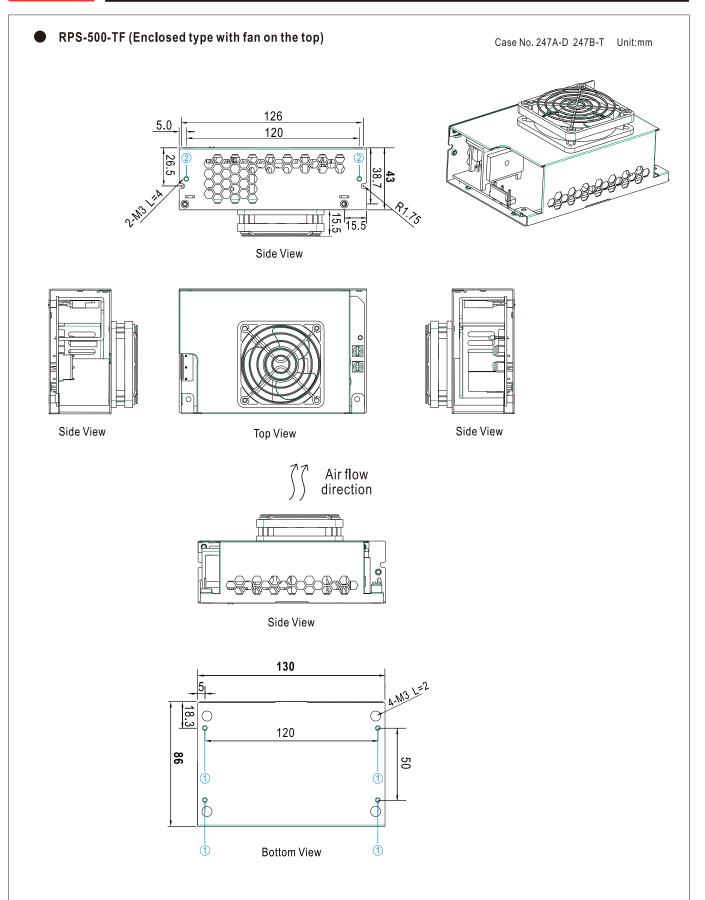


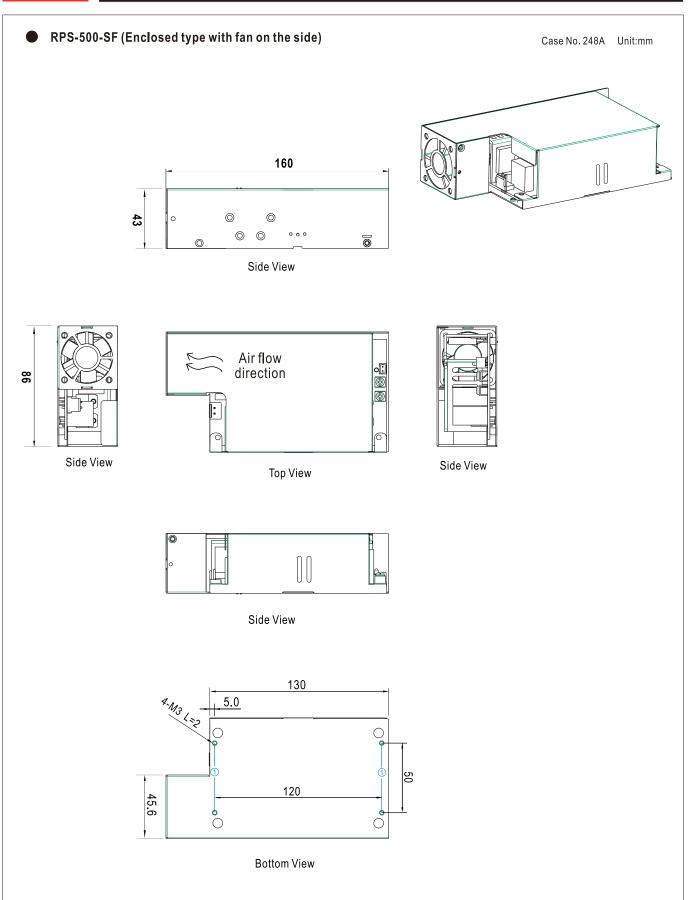



### **※** Mounting Instruction for -C/-TF/-SF Type

Hole No.	Recommended Screw Size	MAX. Penetration Depth L	Recommended mounting torque
1	M3	2mm	4~6Kgf-cm
2	M3	4mm	4~6Kgf-cm



### **X** CONNECTION

AC Input Connector (CN1): JST B3P-VH or equivalent

Pin No.	Assignment	Mating Housing	Terminal
1	AC/N		
2	No Pin	JST VHR or equivalent	JST SVH-21T-P1.1 or equivalent
3	AC/L		or equivalent

### DC Output Connector (CN2,CN3)

Pin No.	Assignment	Output Terminals
CN2	-V	M3.5 Pan HD screw in 2 positions
CN3	+V	Torque to 8 lbs-in(90cNm)max.

HS1,HS2,HS3,HS4 can not be shorted

#### Function Connector(CN11): TKP DH2I-2X2 or equivalent

Pin No.	Assignment	Mating Housing	Terminal
1	-S		
2	+\$	TKP DH2	TKP
3	DC COM	or equivalent	or equivalent
4	PG		

#### Function Connector(CN95): TKP DH2L-2X2 or equivalent

Pin No.	Assignment	Mating Housing	Terminal
1	5Vsb	TI/D DIII0	TKP
2,4	DC COM	TKP DH2 or equivalent	or equivalent
3	PS-ON	3. 343.7410111	3, 344, 4410111

FAN Connector(CN12) : TKP 8812-2 or equivalent (Except for RPS-500-TF/SF)

Pin No.	Assignment	Mating Housing	Terminal
1	DC COM	TKP 2502	TKP 8811
2	+12V	or equivalent	or equivalent

- \*\* Note: 1. The enclosed type (-C/TF/SF type) models are not suitable for configuration within a Class II (without FG) system, but suggested within a Class I (with FG) system.
  - 2. Mounting Instruction for enclosed type.

#### **■** Installation Manual

Please refer to: http://www.meanwell.com/manual.html